

IndiMag[®] Pathogen Kit

Quick Start Protocol

For use with the IndiMag 2 (using 32-well blocks and elution strips)

The IndiMag Pathogen Kit w/o plastics (cat. no. SP947257) can be stored at room temperature (15-25°C). For expiry date information, read the label on the kit box.

Further information and support

- IndiMag Pathogen Kit w/o plastics Handbook: www.indical.com/handbooks
- Technical assistance: support@indical.com

Important notes before starting

- Read the safety information in the IndiMag 2 user manual before use.
- Add Buffer AVE to dissolve carrier RNA as indicated on the tube.
- Add isopropanol (100 %) to Buffer ACB and ethanol (96-100 %) to Buffers AW1 and AW2 before use. See the respective bottle labels for volumes.
- Vortex MagAttract[®] Suspension G for 3 minutes and ensure that it is fully resuspended.
- Equilibrate buffers to room temperature (15-25°C).

For up-to-date licensing information and product-specific disclaimers, see the respective INDICAL kit handbook or user manual. Trademarks: IndiMag[®] and INDICAL[®] (INDICAL BIOSCIENCE); MagAttract[®] (QIAGEN Group, Hilden, Germany). Registered names, trademarks, etc., used in this document, even when not specifically marked as such, are not to be considered unprotected by law. HB-2651-EN-001 03/2025 © 2025 INDICAL BIOSCIENCE GmbH, all rights reserved.

Procedure


1. Label and prepare 32-well blocks (B; columns 2-4), and elution strips (E) according to Table 1 and Figure 1.

Table 1 and Figure 1 (right): Instrument setup and reagent volumes

Column (B)	Item to add	Volume per well
1 Lysate	Lysate*	720 µl
2 Wash 1	Buffer AW 1	700 µl
3 Wash 2	Buffer AW 2	700 µl
4 Wash 3	Ethanol (96-100 %)	750 µl

Elution strip (E)	Item to add	Volume per well
E Elution	Buffer AVE	100 µl

* Includes 20 µl Proteinase K, 200 µl sample and 500 µl Buffer VXL mixture

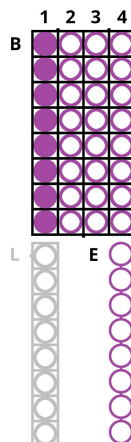

2. Prepare Buffer VXL mixture according to Table 2.

Table 2: Buffer VXL mixture preparation

Reagent	Reactions			
	1	8	24	48
Buffer VXL	100 µl	800 µl	2.4 ml	4.8 ml
Buffer ACB	400 µl	3.2 ml	9.6 ml	19.2 ml
MagAttract Suspension G	25 µl	200 µl	0.6 ml	1.2 ml
Carrier RNA (1 µg/µl)	1 µl	8 µl	24 µl	48 µl

3. Pipet 20 µl Proteinase K into the bottom of the first column of the 32-well locks and add 200 µl sample according to Table 1 and Figure 1 (B1; marked in purple).

Note: If working with insufficient volume of sample, add PBS, 0.9 % NaCl or nuclease-free water to achieve a total sample volume of 200 µl.

4. Mix Buffer VXL mixture thoroughly for 30 sec and add 500 µl Buffer VXL mixture to each sample in the 32-well blocks B1; marked in purple).
5. Immediately load the prepared 32-well plates and elution strips into the IndiMag 2, load the rod covers into correct positions and start the appropriate protocol.

Note: The “IndiMag Pathogen 0/Block/Elution” protocol is preinstalled on the IndiMag 2.

Change index

PCard	Version	Change
HB-2651-EN-001	March 2025	Product launch